


 **TECAN.**

---

Instructions for Use for

**infinite 200**

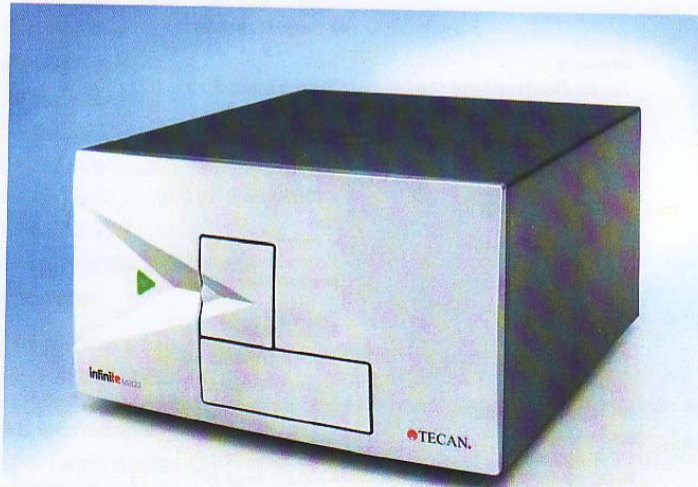

**Fluorimeter/Photometer**

# Features

## **Fluorescence**

- wavelength: Excitation: 230-850 nm,  
Emission: 280-850 nm
- microtiterplates

## **Absorbance**

- wavelength 230-1000 nm
- microtiterplates
- cuvette

Temperatur control: 5°C above ambient temp to 42°C

Kinetic measurements

Wavelength scan

# Fluorescence intensity system

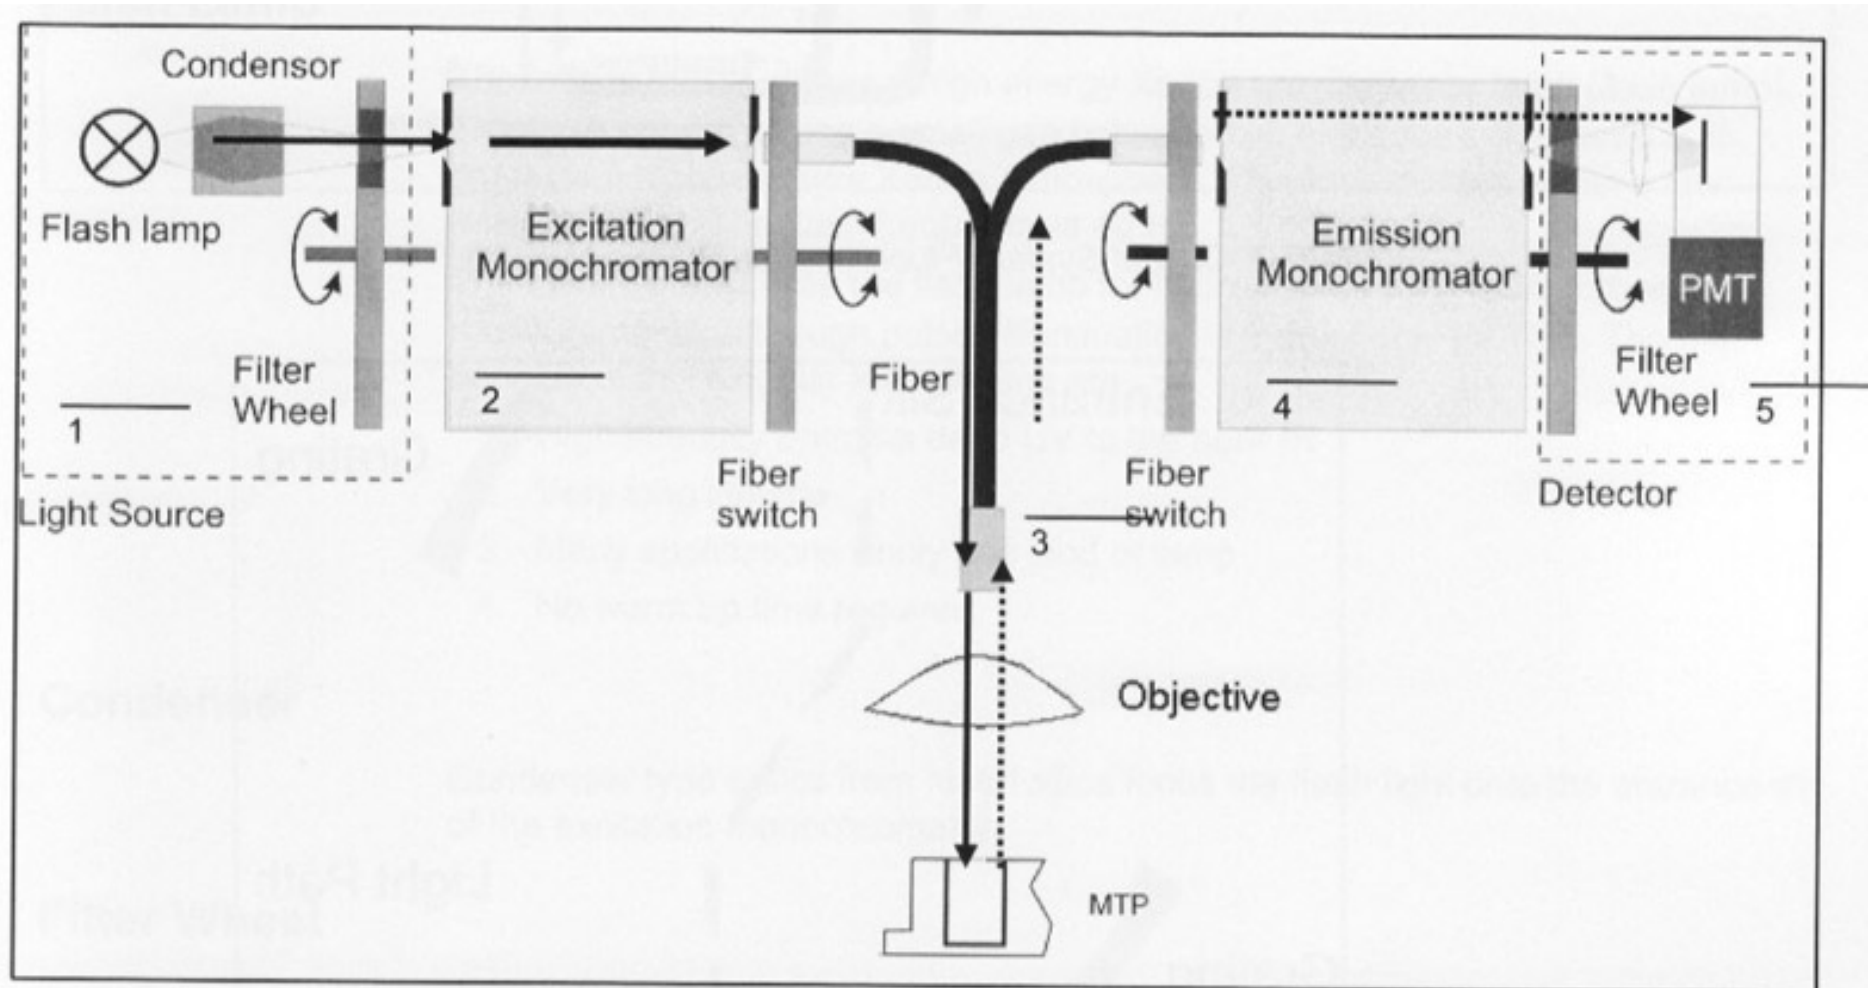


Figure 5-1 Optical System Fluorescence Top

# Absorbance intensity system

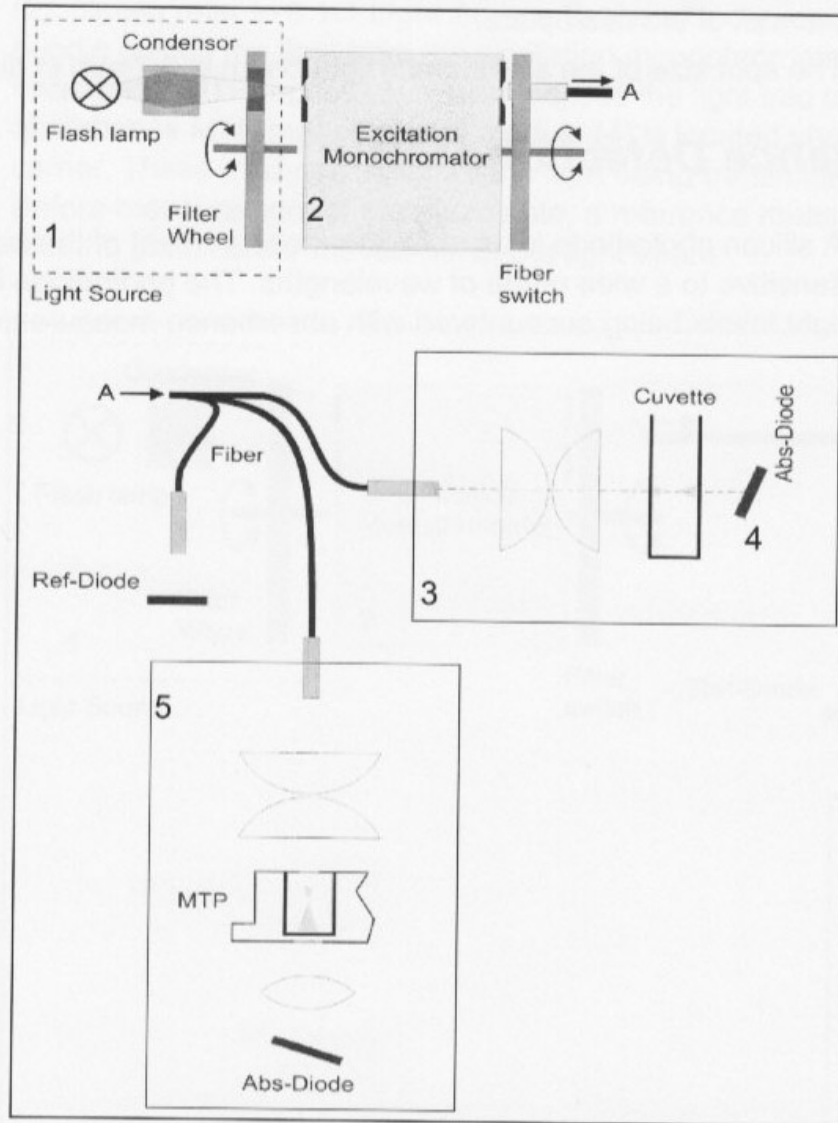


Figure 5-7: Optical System of the absorbance module of **infinite M200** including the cuvette port

# Movie

[http://www.tecan.com/quad4/monochromator\\_video.htm](http://www.tecan.com/quad4/monochromator_video.htm)